

HOTTINGER BALDWIN MESSTECHNIK



**Electrical
measurement
of mechanical
quantities**

Mounting Instructions

Load Cells for Official Calibration C2A

Contents**Page**

Notes on safety	4
1 Mounting information	4
2 Load introduction	5
3 Connection	5
3.1 Parallel connection of several transducers	6
3.2 Connections using the four-wire technique	6
3.3 Cable extensions	6
3.4 Notes on cable routing	7
4 Special information	7
5 Technical data	8
6 Dimensions	9

Notes on safety

The C2A... Load Cells can be used as machine components (e.g. with container weighing). In these cases please note that in order to obtain a high measurement sensitivity the load cells have not been designed with the safety factors usually encountered in machine design. If component fracture may lead to damage to property or injury to persons, safety measures according to the relevant accident prevention regulations (e.g. support against collapse, overload protection) must be taken by the user. In chapter 5 we provide important details in this respect, such as

- save load limit,
- side load limit,
- breaking loads and
- permissible dynamic loads.

The electronic system processing the measurement signal should be designed such that no consequential damage occurs as the result of a failure of the measurement signal.

1 Mounting information

- Handle the transducer carefully.
- Do not overload the transducer (e.g. by unevenly distributed loads); if necessary, provide overload protection (e.g. supports).
- The transducer seating must be horizontal, even and, together with the transducer mounting surface, it must be absolutely clean.
- Each transducer should be bridged by a copper wire (approx. 50mm²) during or immediately after installation, so that no welding currents can flow across the transducer.
- Dust, dirt and other foreign matter must not be allowed to collect so that the deflection of the transducer is impaired, leading to possible erroneous measurements.

2 Load introduction

When applied in weighing equipment, load cells are subjected to unwanted side forces and moments. These may arise from deformation of the loaded weighing machine structure or through thermal strains. To keep the effects on the measurement resulting from these forces and moments as low as possible, HBM supplies pendle supports and elastomer bearings as load introduction components. Both types of load introduction components enable a design with a degree of horizontal movement with respect to the load cells. A deflection causes a reactive force which attempts to restore the weighing machine to its original position. With the pendle supports this restoring force is proportional to the deflection and the current loading and with elastomer bearings it is proportional to the deflection. This means that a different characteristic is obtained, particularly under partial loading conditions.


The elastomer bearing also possesses higher damping in the horizontal and vertical directions. In both cases no stay rods are needed. It is sufficient to limit the horizontal movement of the weighing machine structure using mechanical stops (take note of s_{\max} in chapter 6).

3 Connection

Strain-gauge based load cells can be connected to:

- carrier frequency or
- DC-measuring amplifiers.

The transducer connection is implemented using the six-wire technique. The connection assignment can be taken from the following illustration.

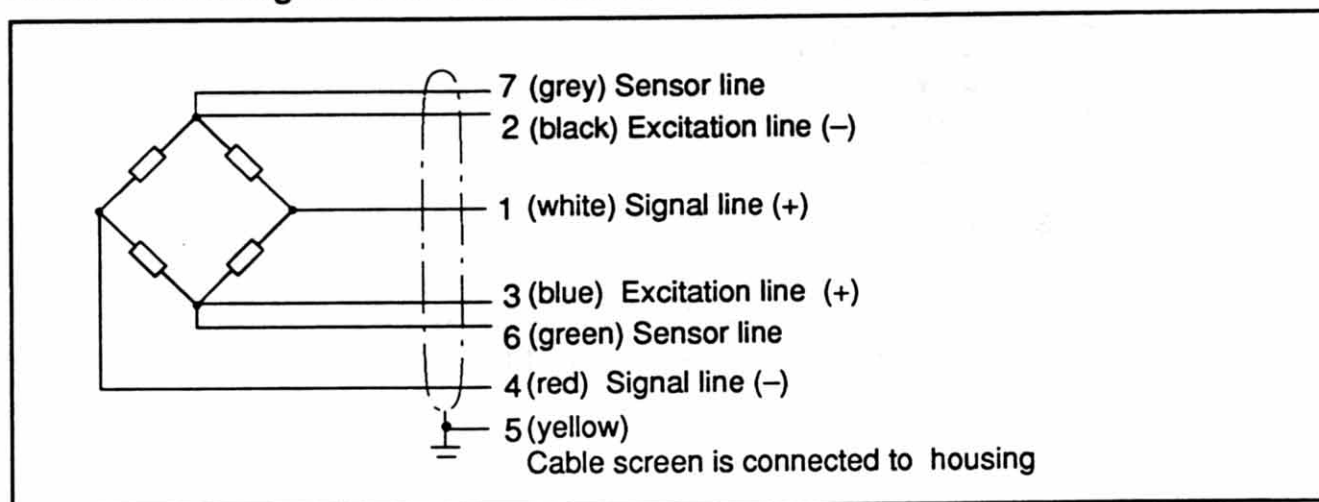

Electrical and magnetic fields often induce interference voltages in the measurement circuit.

Therefore:

- Use screened low-capacitance measurement cables only (HBM cables satisfy this criterion).
- Do not route the measuring cable parallel to power and control lines. If this is not possible, protect the measurement cable, e.g. with steel conduit.
- Avoid the stray fields of transformers, motors and contactors.

3.1 Parallel connection of several transducers

Transducers can be wired in parallel by joining the transducer cable core ends of the same colour.

Caution: Overloading in a single load cell can no longer be detected from the output signal.

3.2 Connections using the four-wire technique

With connections to amplifiers using the four-wire technique the cores BU (blue) and GN (green) should be connected together, as should BK (black) and GR (grey). Please take in account that this causes deviations to the sensitivity and the temperature coefficient of sensitivity that this causes.


3.3 Cable extensions

Cable extensions must be screened and of low capacitance. We recommend the use of HBM cables which satisfy these requirements. With cable extensions it should be ensured that a proper connection is provided with low contact resistances and good insulation.

When using the six-wire technique, the effects of resistance changes in the extension cable are compensated. If you extend the cable with the four-wire technique, the sensitivity deviation can be rectified by adjustment. Temperature effects though are only compensated with the operation using the six-wire technique.

3.4 Notes on cable routing

The load cell connecting cable should be routed so that any condensed water or dampness forming on the cable can drip off. It must not be led to the load cell. In addition, it must be ensured that no dampness can penetrate the open end of the cable.

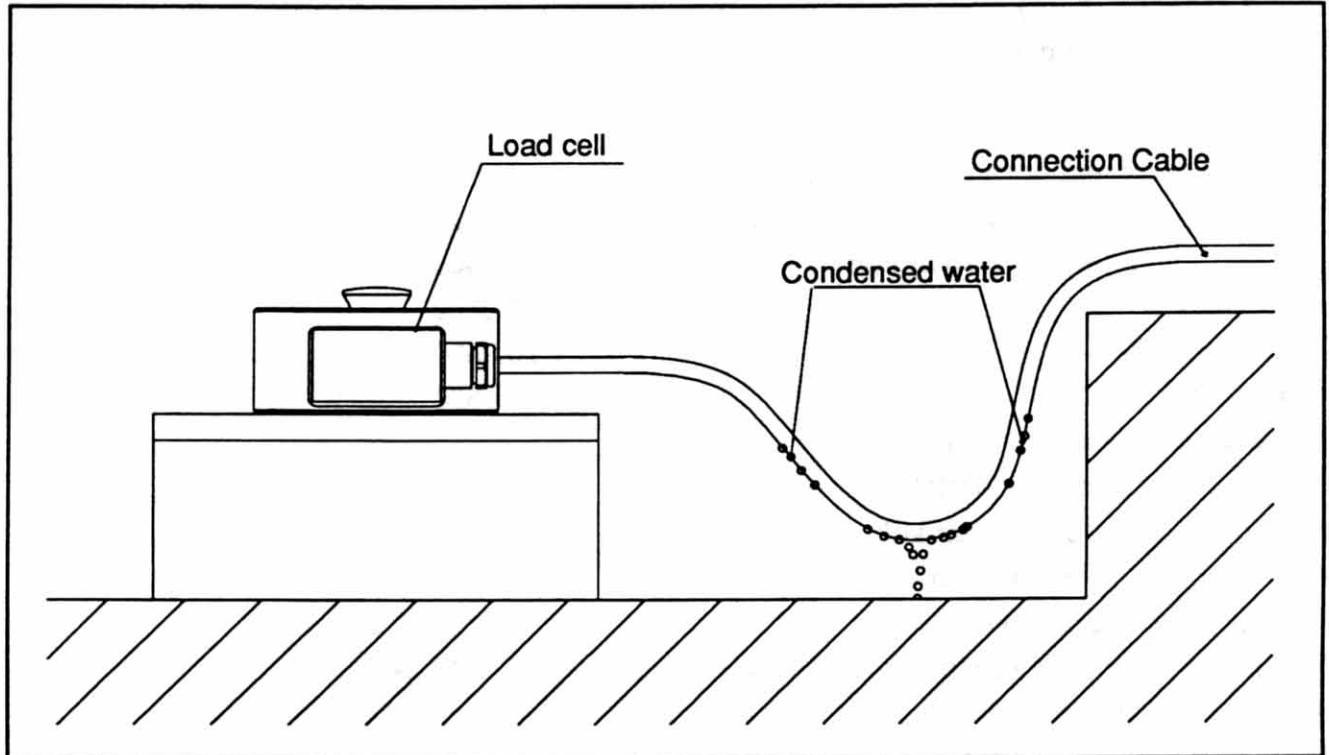

4 Special information

The C2A transducers are produced entirely from non-rusting materials (see Chapter 5). In cases of doubt the resistance to aggressive ambient conditions should be checked by the user.

5 Technical data


Type		C2AD1	C2AC3
Accuracy class to OIML R60		D1	C3
Max. number of load cell intervals (n_{LC})		1000	3000
Rated capacity (E_{max})	t	1, 2, 5, 10	
Min. load cell verification interval (v_{min})	% of rat. capacity	0.0286	0.0100
Rated output	mV/V	2	
Tolerance on rated output	%	<±0.1000	<±0.0500
Temperature effect on sensitivity ¹⁾	%/10K	<±0.0500	<±0.0080
Temperature effect on zero signal	%/10K	<±0.0400	<±0.0140
Hysteresis ¹⁾	%	<±0.0500	<±0.0180
Non linearity ¹⁾	%	<±0.0500	<±0.0170
Creep in 30 min	%	<±0.0500	<±0.0167
Input resistance (black-blue)	Ω	350...450	
Output resistance (red-white)	Ω	356±1.5	356±0.12
Nominal range of excitation volt.	V	0.5...12	
Max. permissible excitation volt.	V	18	
Reference temperature	°C [°F]	+ 23 [+73]	
Nominal temperature range	°C [°F]	-10...+40 [+15...105]	
Service temperature range	°C [°F]	-30...+70 [-20...+160]	
Storage temperature range	°C [°F]	-50...+85 [-60...+185]	
Safe load limit	% of rat. capacity	150	
Breaking load	% of rat. capacity	300	
Side load limit	% of rat. capacity	50	
Permissible dynamic load (Vibration amplitude to DIN 50100)	% of rat. capacity	100 ²⁾	
Deflection at rated load, approx. (± 15%)	mm	0.15; 0.15; 0.17; 0.2	
Weight, approx.	kg	1.7; 1.8; 1.8; 1.8	
Protection class to EN 60529 (IEC529)		IP 67 (Test conditions:100h at 1m water column)	
Materials		Rust resistant Nickel plated brass Silicone	
Measuring body			
Cable gland			
Cable sheath			

¹⁾ The data for deviation of non linearity, hysteresis and temperature effect on rated output are typical values. The sum of these data meets the requirements according to OIML R60.

²⁾ 70% with C2A./10t

6 Dimensions


C2A /1...10t, Pendle support ZPS25/66 and Pendle support upper part EPO3R/ST

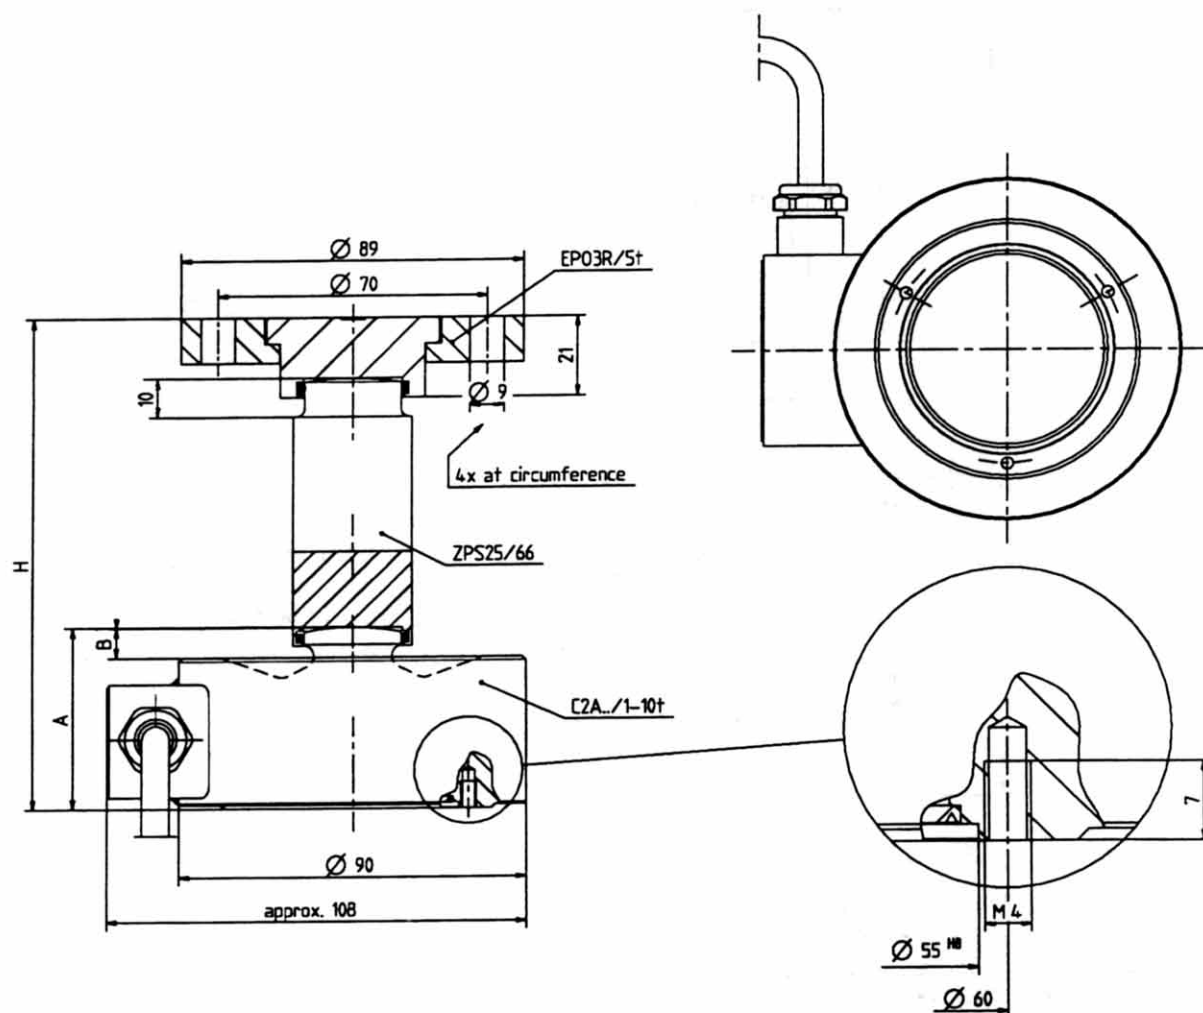

F_R : Restoring force for 1mm sideways deflection

S_{max} : Maximum permissible sideways deflection at rated capacity

Rated capacity	A	B	Pendle support	H	S_{max} (mm)	F_R (% of applied load)
1t	48	10	ZPS25/66	130	± 5	1
2t	48	10	ZPS25/66	130	± 5	1.5
5t	48	8	ZPS25/66	130	± 5	1.7
10t	53	8	ZPS25/66	135	± 5	2.2

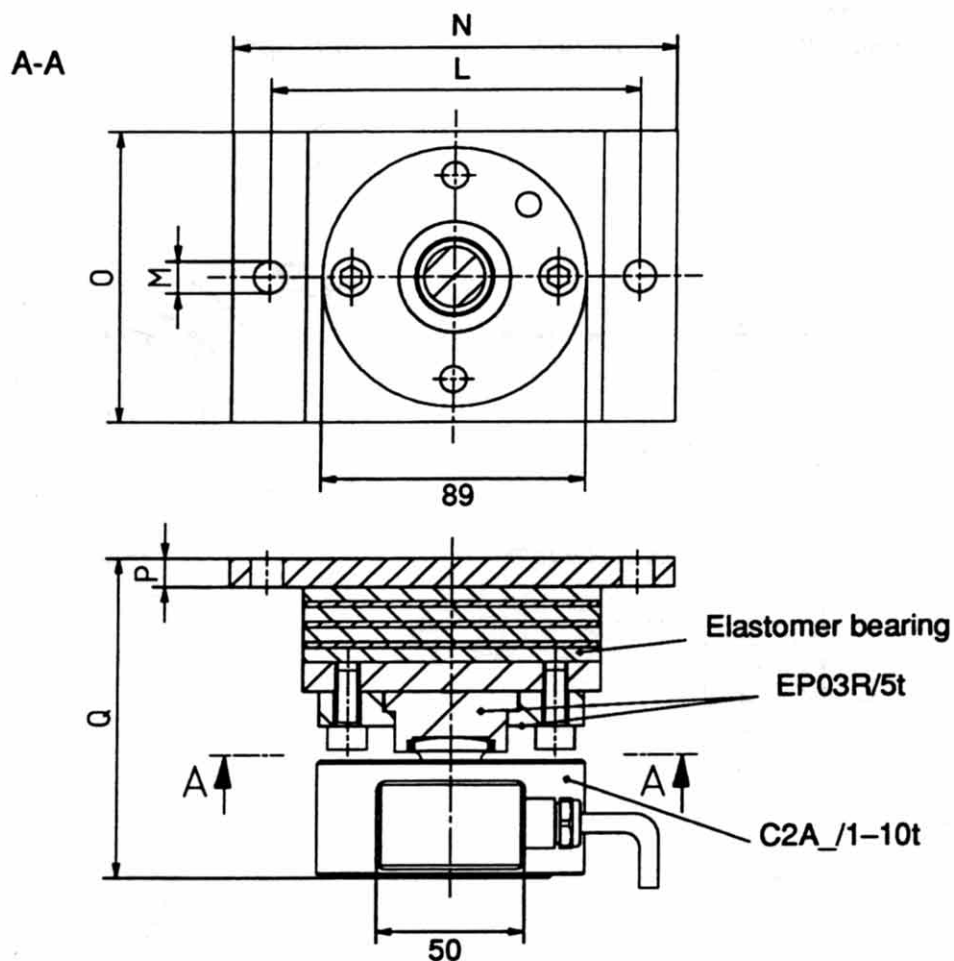C2A /1...10t, Elastomer Bearing ZELB and Pendle support upper part EPO3R/ST

F_R : Restoring force for 1mm sideways deflection

$S_{max.}$: Maximum permissible sideways deflection at rated capacity

Rated capacity	Elastomer-bearings	L	M	N	O	P	Q	S_{max} (mm)	F_R (N)
1t	ZELB/2t	100	9	120	60	10	103	± 4.5	400
2t	ZELB/2t	100	9	120	60	10	103	± 4.5	400
5t	ZELB/5t	125	11	150	100	10	110	± 8	620
10t	ZELB/10t	175	13	200	100	12	124	± 9.5	810

Accessories (not included in the supply):

Pendle support ZPS, Pendle support upper part EPO3R and Elastomer bearing ZELB.



HOTTINGER BALDWIN MESSTECHNIK GMBH
Postfach 10 01 51 • 64 201 Darmstadt 1
Im Tiefen See 45, 64 293 Darmstadt
Tel.: (0 61 51) 8 03-0 • Telefax: (0 61 51) 89 48 96

Modifications reserved. All details describe our products in general form.
They are not to be understood as express warranty and do not constitute
any liability whatsoever.

wt 07.95 – 0.5 HBM